


Traceability Chart


หมายเลขเอกสาร :		แก้ไขที่ : 0
DRAF <i>ช. ๙๙๙๙</i>	CHECK <i>Asl</i>	APPROVE <i>ว.ล.</i>
Date :	Date :	Date :

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)
 Accreditation No. : Calibration No. 0116
 Calibration Procedure : WL-M008 Pin, Plug, Cylindrical gauge
 Calibration Scope : Size 0.5 mm to 125 mm


National Metrology Institute (NMI)

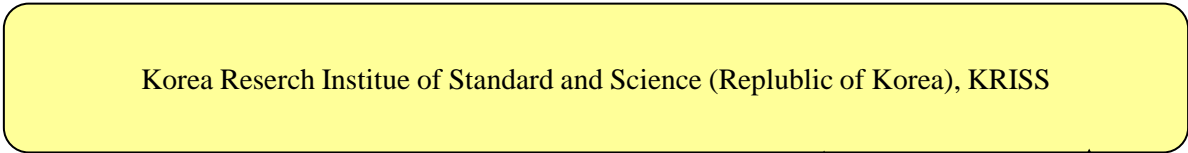

Refernce Standards



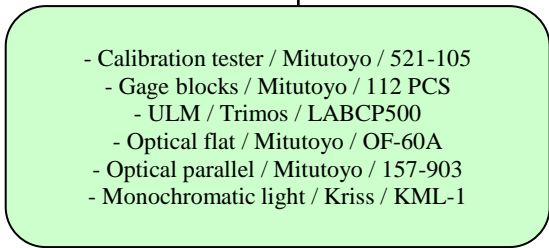


SICT Equipment

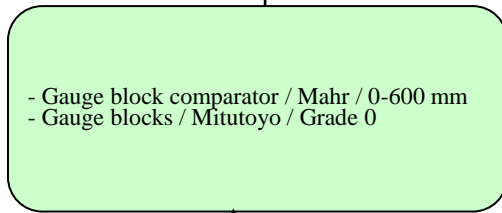


KTL Equipment

TKCC, Working Standards

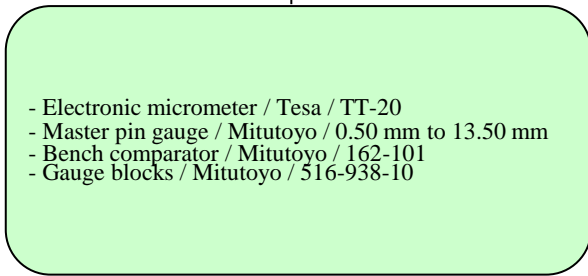

Customer's Equipment

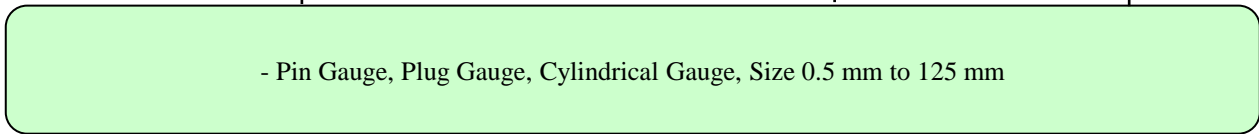

Remark :

- NMI : National Matrology Institute
- KRISS : Korea Reserch Institue of Standard and Science (Replublic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd. (KC01-018)
- KTL : Korea Testing Laboratory (KC01-028)