


Traceability Chart

หมายเลขเอกสาร :		แก้ไขที่ : 0
DRAF <i>Stan</i>	CHECK <i>TL</i>	APPROVE <i>ว.ส.ิ</i>
Date :	Date :	Date :

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)
 Accreditation No. : Accredited by TLAS Calibration No. 0116
 Calibration procedure : WL-E026 EARTH CONTINUITY TESTER
 Calibration scope for : RESISTANCE TEST (AC) @ 45 Hz to 60 Hz
 50 to 500 mΩ @ 5 A to 60 A 4W
 50 to 500 mΩ @ 5 A to 60 A 2W

Traceable to National Metrology Institute (NMI)

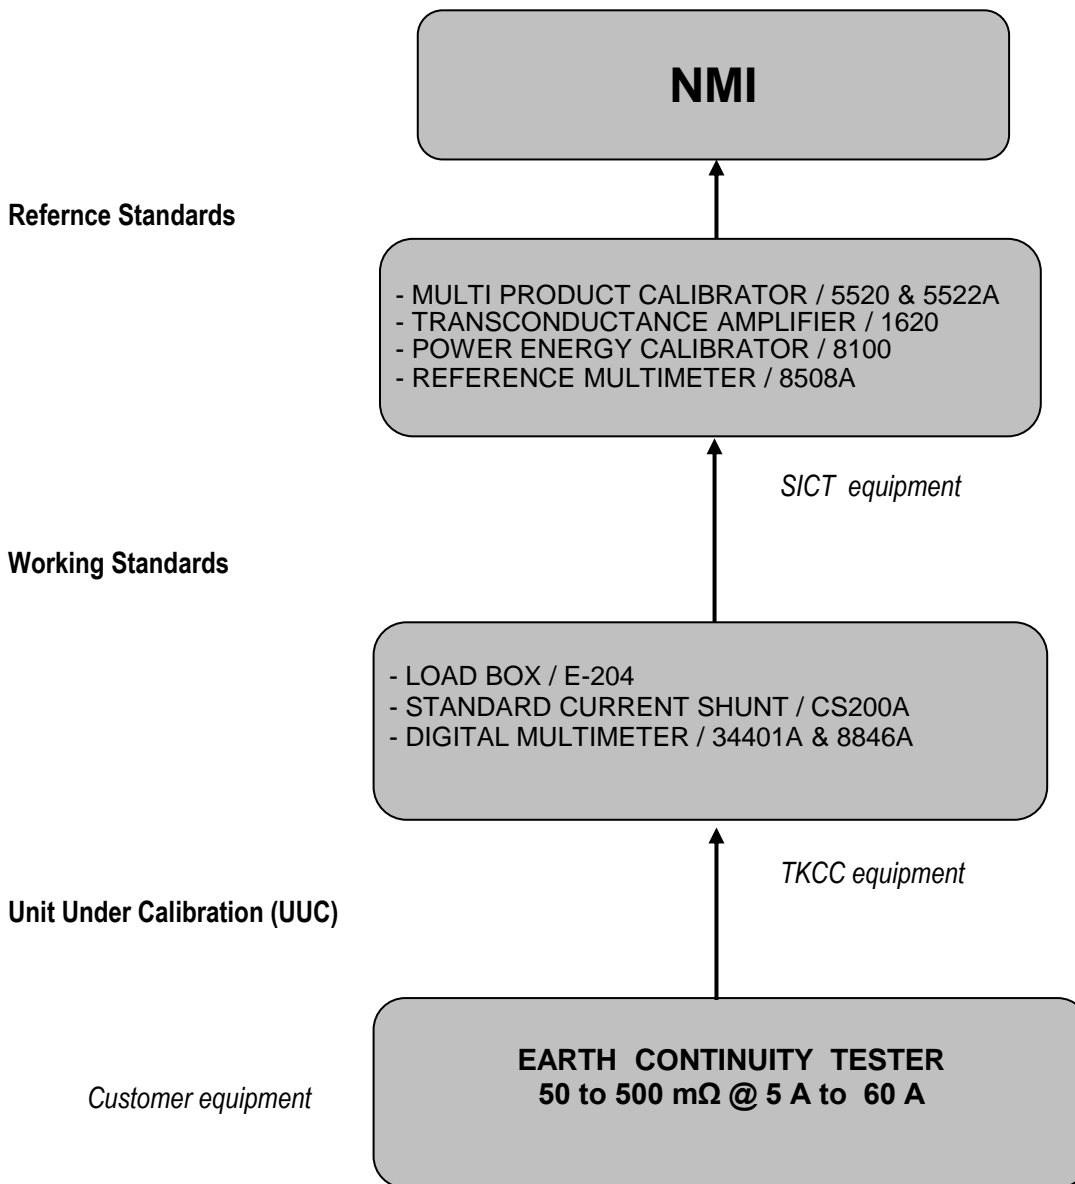

Remark :

- NMI : National Metrology Institute
- KRISS : Korea Research Institute of Standard and Science (Republic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd.