


Traceability Chart

หมายเลขเอกสาร :		แก้ไขที่ : 0
DRAF <i>[Signature]</i> Date :	CHECK <i>[Signature]</i> Date :	APPROVE <i>[Signature]</i> Date :

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)
 Accreditation No. : Accredited by TLAS Calibration No. 0116
 Calibration procedure : WL-E002 AC VOLTAGE MEASURING INSTRUMENT CALIBRATION
 Calibration scope for : 1 mV to 3.3 V @ 45 Hz to 100 kHz
 3.3 mV to 33 V @ 45 Hz to 90 kHz
 33 mV to 330 V @ 45 Hz to 20 kHz
 330 mV to 1020 V @ 45 Hz to 8 kHz

Traceable to National Metrology Institute (NMI)

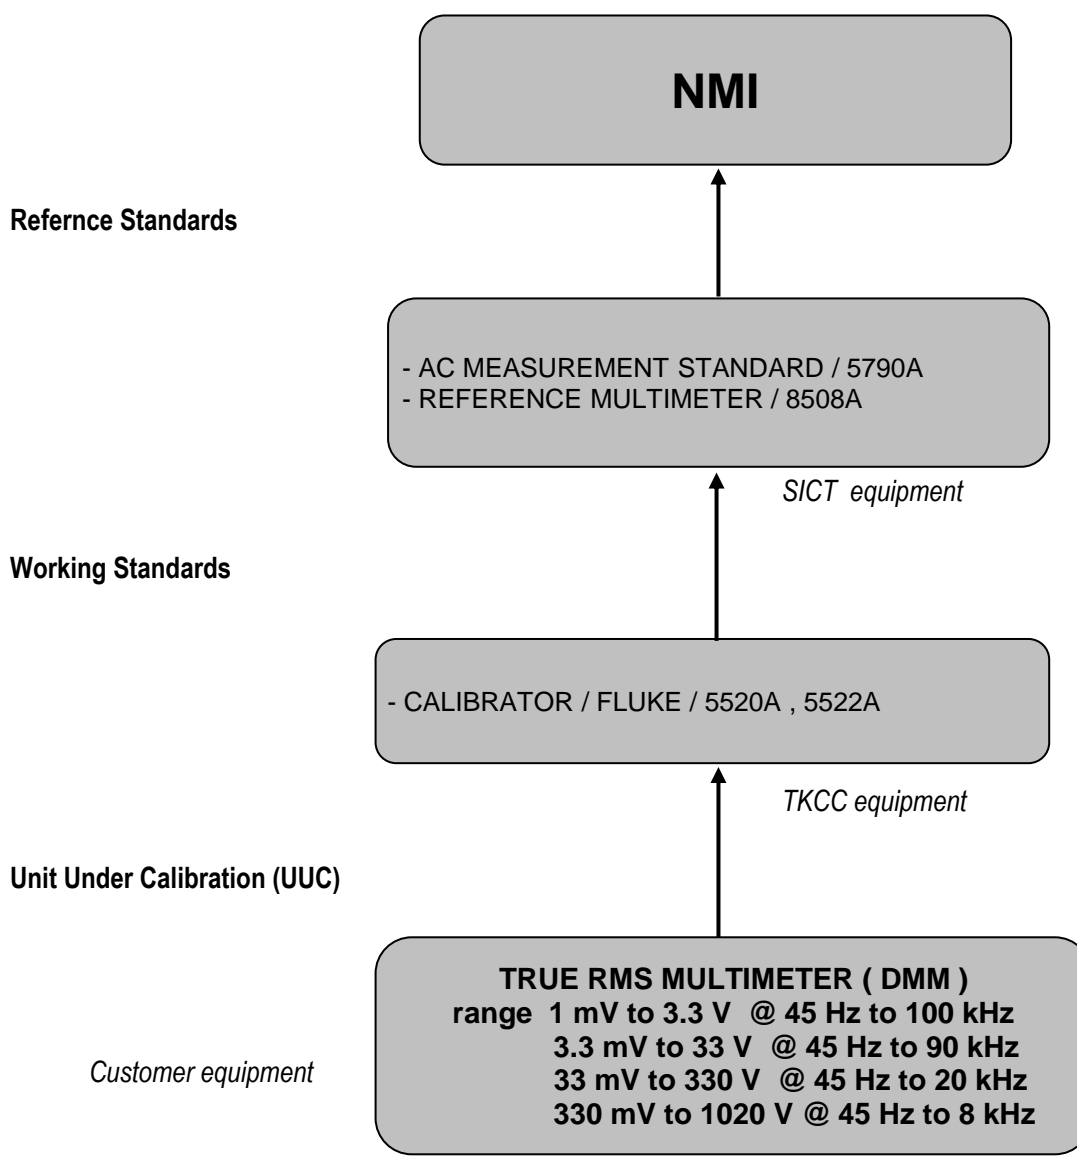

Remark :

- NMI : National Metrology Institute
- KRISS : Korea Research Institute of Standard and Science (Republic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd.