





Traceability Chart

หมายเลขเอกสาร :		แก้ไขที่ : 0
DRAF	CHECK	APPROVE
		
Date :	Date :	Date :

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)
 Accreditation No. : Accredited by TLAS Calibration No. 0116
 Calibration procedure : WL-E004 AC CURRENT MEASURING INSTRUMENT CALIBRATION
 Calibration scope for : 29 uA to 3 A @ 45 Hz to 1 kHz
 3 A to 20 A @ 45 Hz to 90 kHz
 20 A to 50 A @ 50 Hz to 400 Hz

Traceable to National Metrology Institute (NMI)

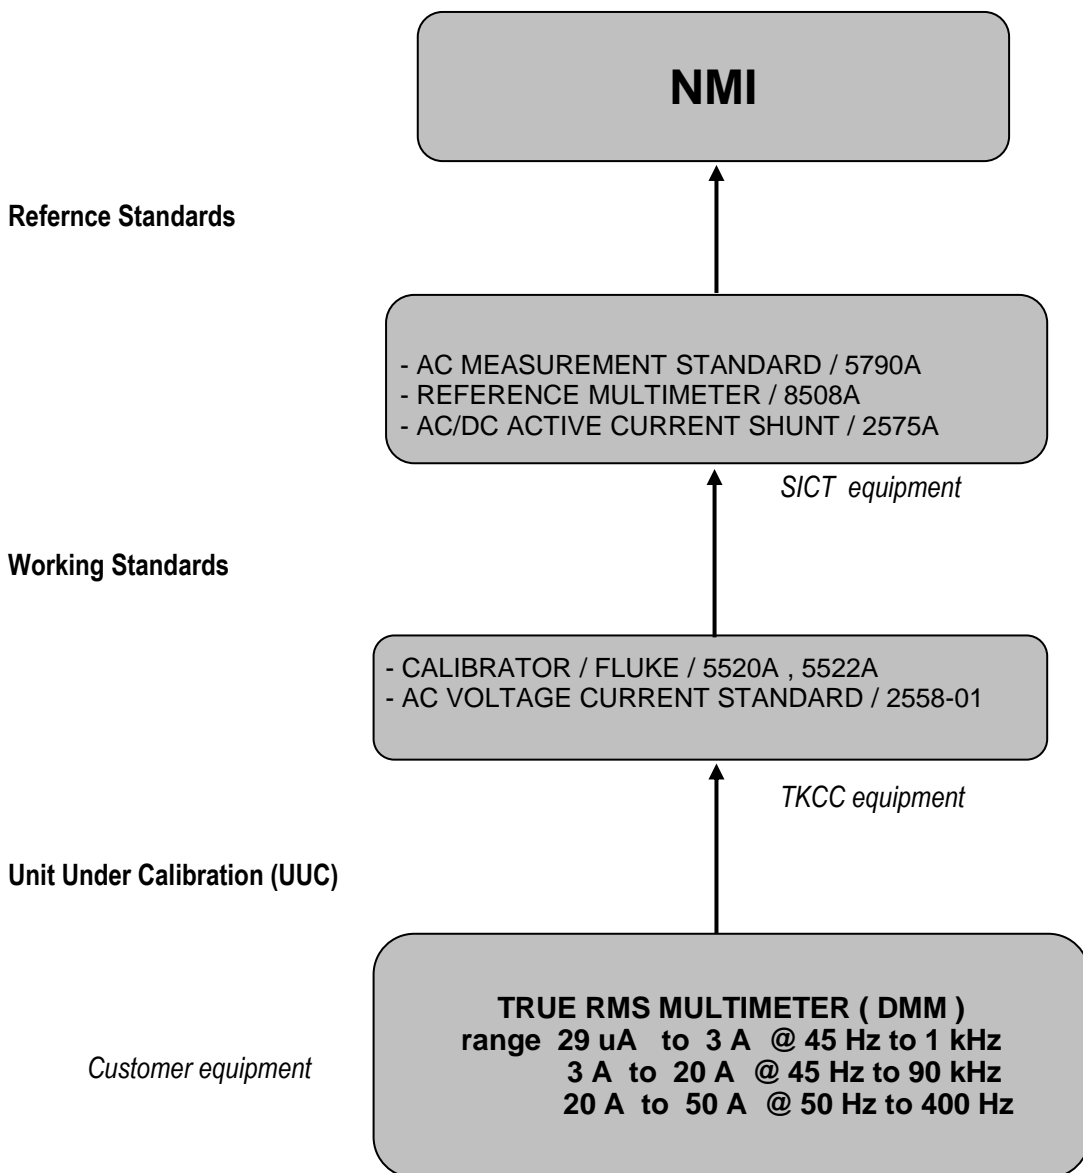

Remark :

- NMI : National Matrology Institute
- KRISS : Korea Reserch Institue of Standard and Science (Replublic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd.