


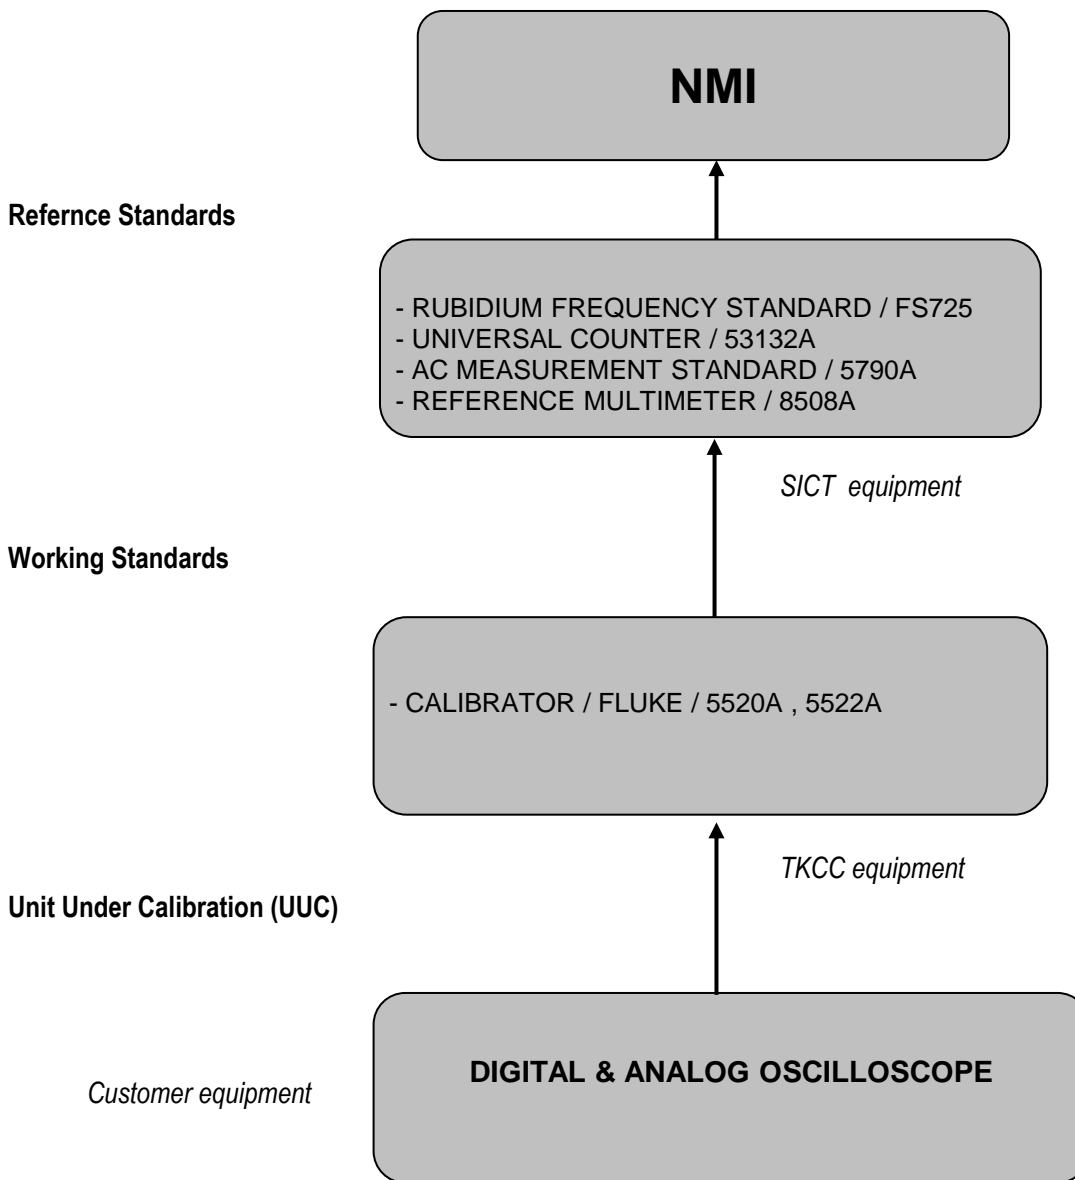


Traceability Chart

หมายเลขเอกสาร :		แก้ไขที่ : 0
DRAF  Date :	CHECK  Date :	APPROVE  Date :

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)
 Accreditation No. : Accredited by TLAS Calibration No. 0116
 Calibration procedure : WL-E023 DIGITAL & ANALOG OSCILLOSCOPE
 Calibration scope for : DC coupling 1 MΩ (2mV to 20V) ;DC coupling 50 Ω (2mV to 1V)
 AC coupling 1 MΩ (2mV to 20V) ;AC coupling 50 Ω (2mV to 1V)
 Horizontal deflection (10ns to 5s)
 Leveled Sine Wave 5 mVp-p to 600 mVp-p at 50kHz to 600MHz

Traceable to National Metrology Institute (NMI)



Remark :

- NMI : National Metrology Institute
- KRISS : Korea Research Institute of Standard and Science (Republic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd.