


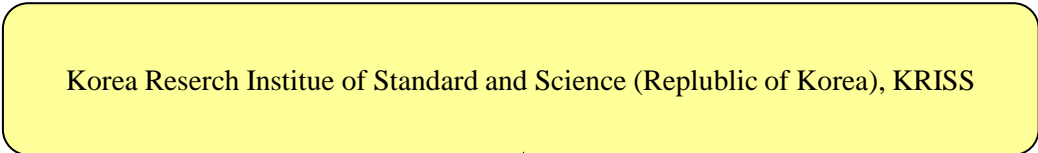


# Traceability Chart


หมายเลขเอกสาร :	SL-M	แก้ไขที่ :	0
DRAF	CHECK	APPROVE	
			
Date :	Date :	Date :	

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)  
 Accreditation No. : Calibration No. 0116  
 Calibration Procedure : WL-M034 Pressure Measuring Instrument (Hydraulic type)  
 Calibration Scope : Pressure measuring device (Hydraulic type). Range 0 kPa to 70 Mpa (700 bar)

National Metrology Institute (NMI)




Reference Standards

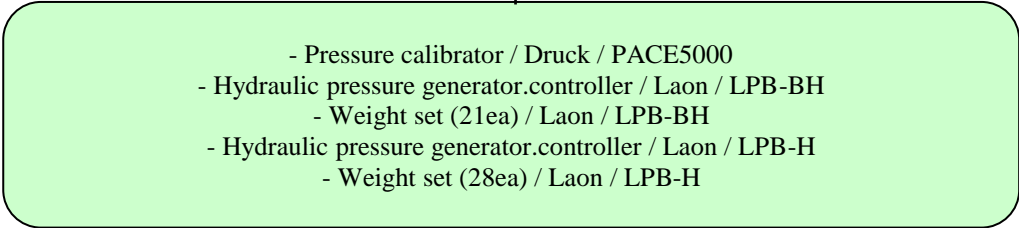


SICT Equipment

TKCC, Working Standards

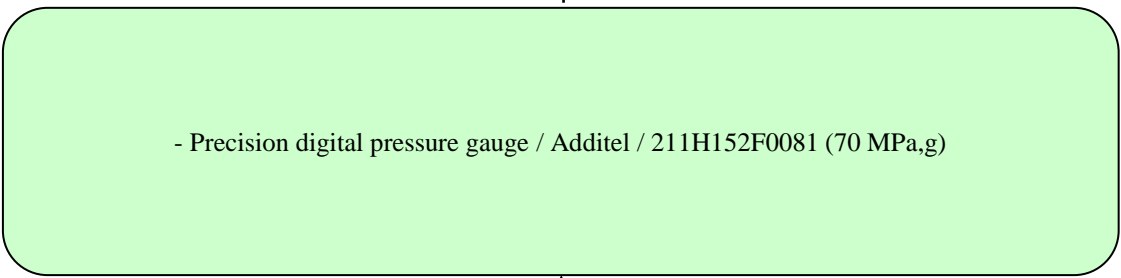

Customer's Equipment

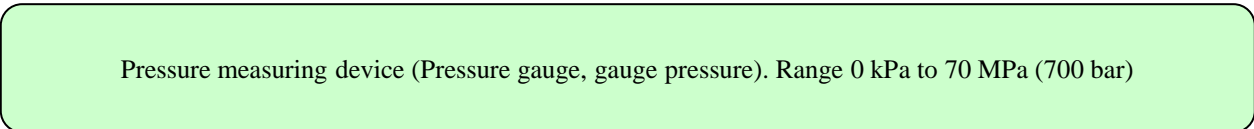

Remark :

- NMI : National Matrology Institute
- KRISS : Korea Reserch Institue of Standard and Science (Replublic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd. (KC01-018)