


# Traceability Chart

หมายเลขเอกสาร :		แก้ไขที่ : 0
DRAF <i>Rowit</i>	CHECK <i>TL.</i>	APPROVE <i>Rowit</i>
Date :	Date :	Date :

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)  
 Accreditation No. : Accredited by TLAS Calibration No. 0116  
 Calibration procedure : WL-E010 THERMOCOUPLE TEMPERATURE INDICATORS  
 Calibration scope for :  
 -190 °C to 1 200 °C ( K-TYPE )  
 -190 °C to 350 °C ( T-TYPE )  
 -190 °C to 900 °C ( J-TYPE )

## Traceable to National Metrology Institute (NMI)

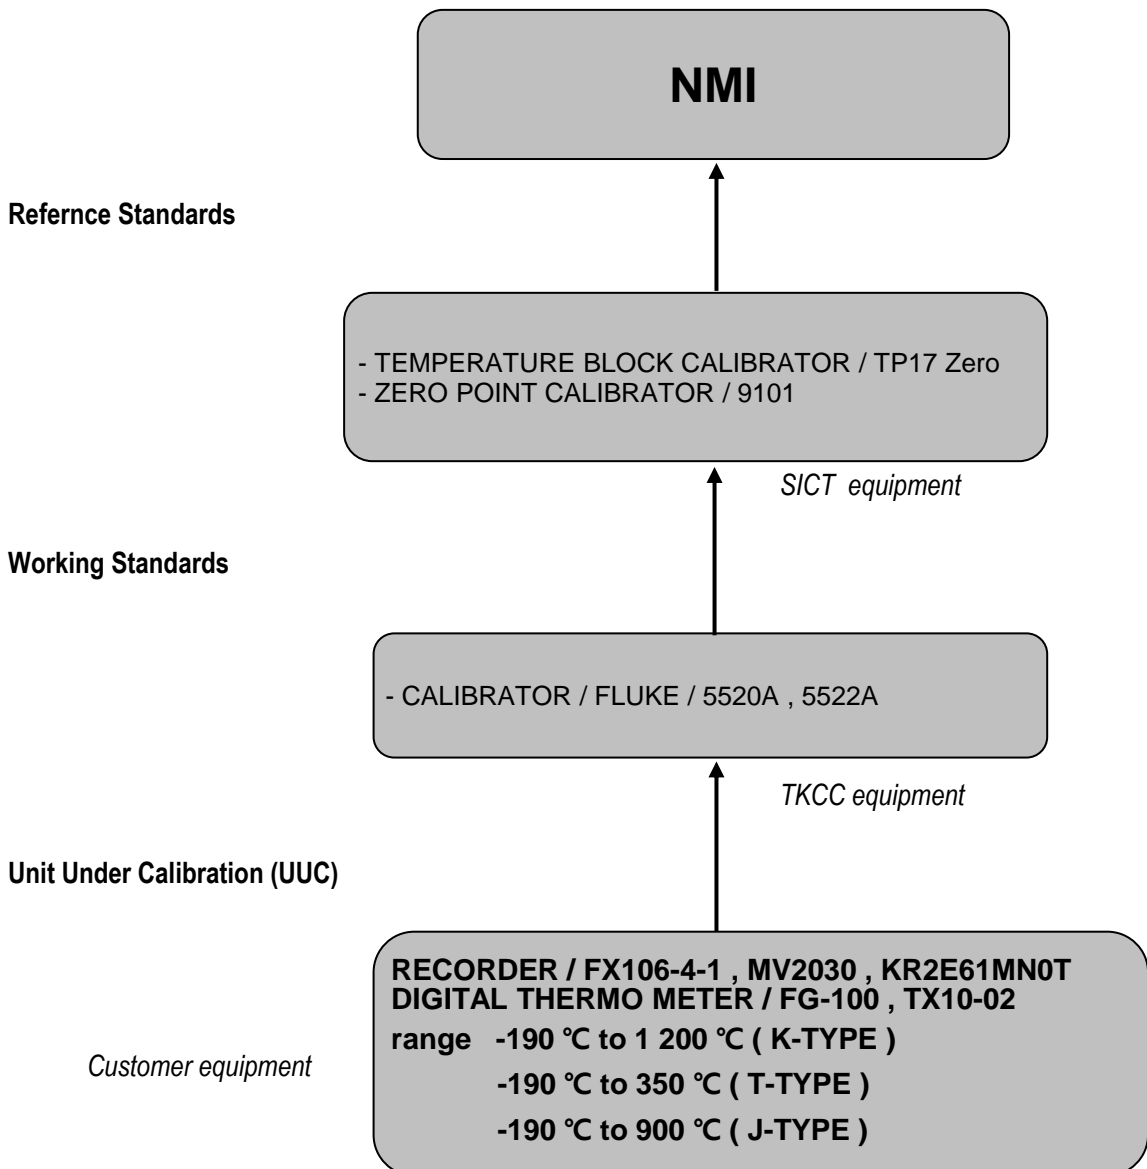

Remark :

- NMI : National Metrology Institute
- KRISS : Korea Research Institute of Standard and Science (Republic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd.