


Traceability Chart

หมายเลขเอกสาร :		แก้ไขที่ : 0
DRAF <i>Powit</i>	CHECK <i>TL.</i>	APPROVE <i>...</i>
Date :	Date :	Date :

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)
 Accreditation No. : Accredited by TLAS Calibration No. 0116
 Calibration procedure : WL-E018 HUMIDITY / TEMPERATURE CONTROLLED CHAMBER
 Calibration scope for : Temperature -40 °C to 200°C
 @ Ref. T(temp.) at 20 °C to 80 °C
 20% to 95%

Traceable to National Metrology Institute (NMI)

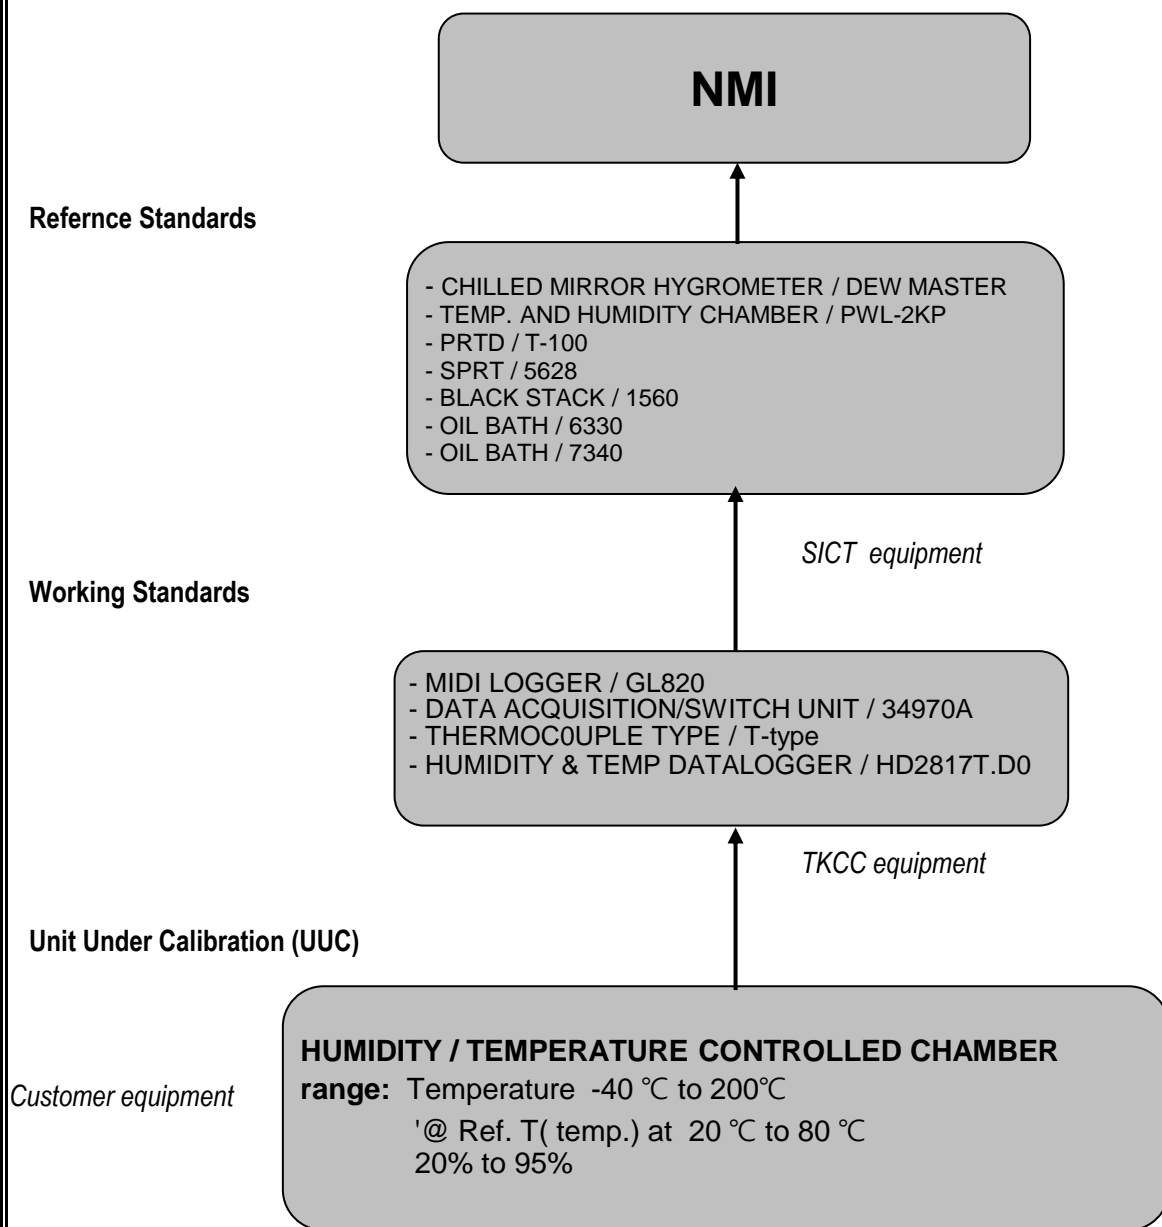

Remark :

- NMI : National Metrology Institute
- KRISS : Korea Research Institute of Standard and Science (Republic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd.