


# Traceability Chart

|                                |                               |                                  |
|--------------------------------|-------------------------------|----------------------------------|
| หมายเลขเอกสาร :                |                               | แก้ไขที่ : 0                     |
| DRAF<br><i>Pawit</i><br>Date : | CHECK<br><i>TL.</i><br>Date : | APPROVE<br><i>W.S.</i><br>Date : |

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)  
 Accreditation No. : Accredited by TLAS Calibration No. 0116  
 Calibration procedure : WL-E028 Thermo-hygrograph  
 Calibration scope for : Temperature '0 °C to 50 °C  
 Humidity 20 %RH to 95 %RH at 23°C to 40°C

## Traceable to National Metrology Institute (NMI)

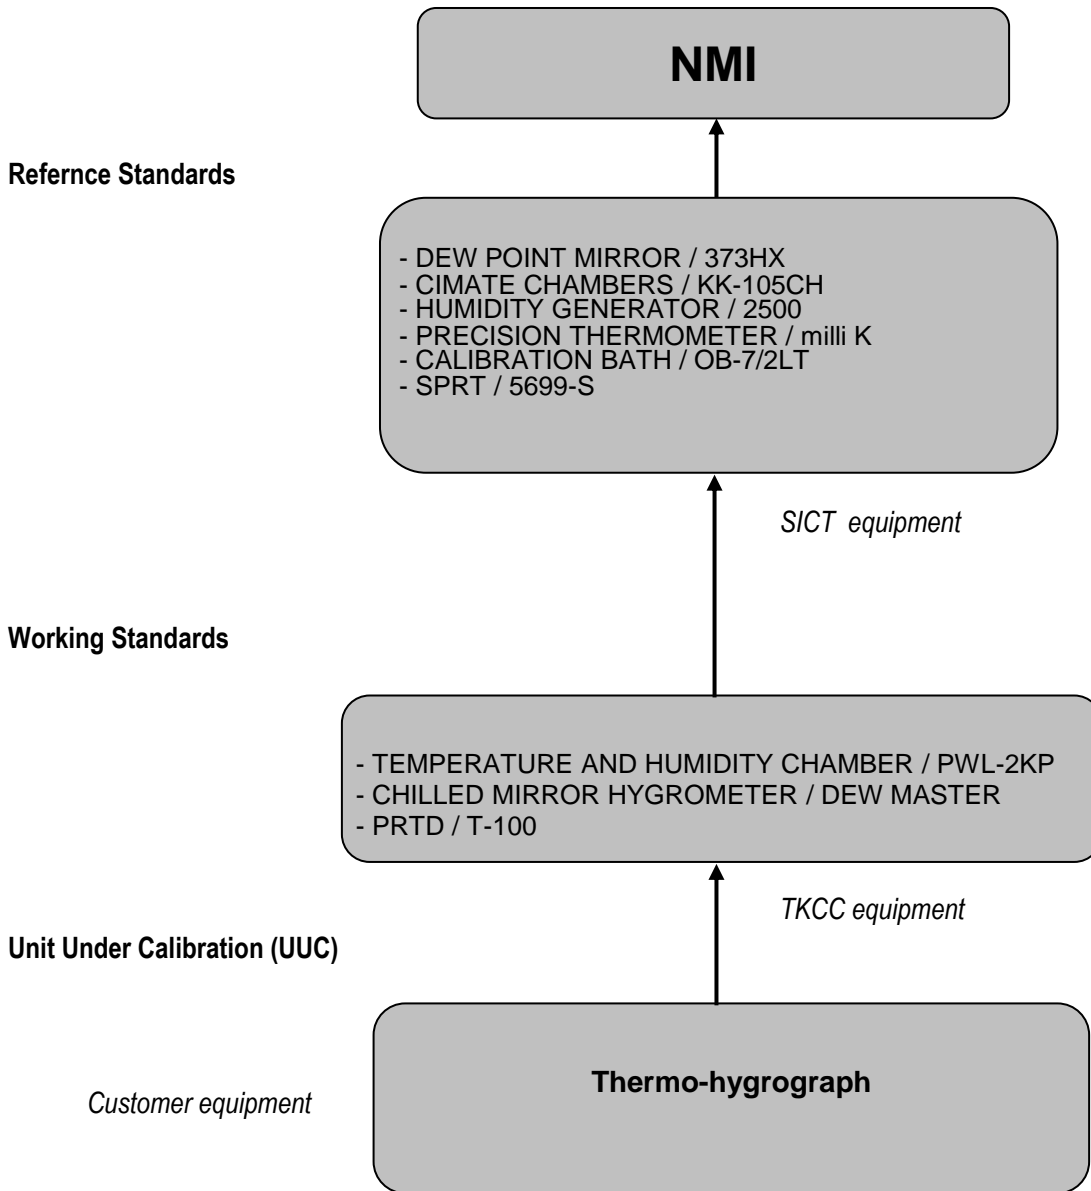

Remark :

- NMI : National Metrology Institute
- KRISS : Korea Research Institute of Standard and Science (Republic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd.