


Traceability Chart

| | | |
|--------------------------------|-------------------------------|---|
| หมายเลขเอกสาร : | | แก้ไขที่ : 0 |
| DRAF <i>Pawit</i> Date : | CHECK <i>TL.</i> Date : | APPROVE <i>[Signature]</i> Date : |

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)
 Accreditation No. : Accredited by TLAS Calibration No. 0116
 Calibration procedure : WL-E038 Digital thermometer with sensor RTD
 Calibration scope for : Temperature -39 to 600 °C

Traceable to National Metrology Institute (NMI)

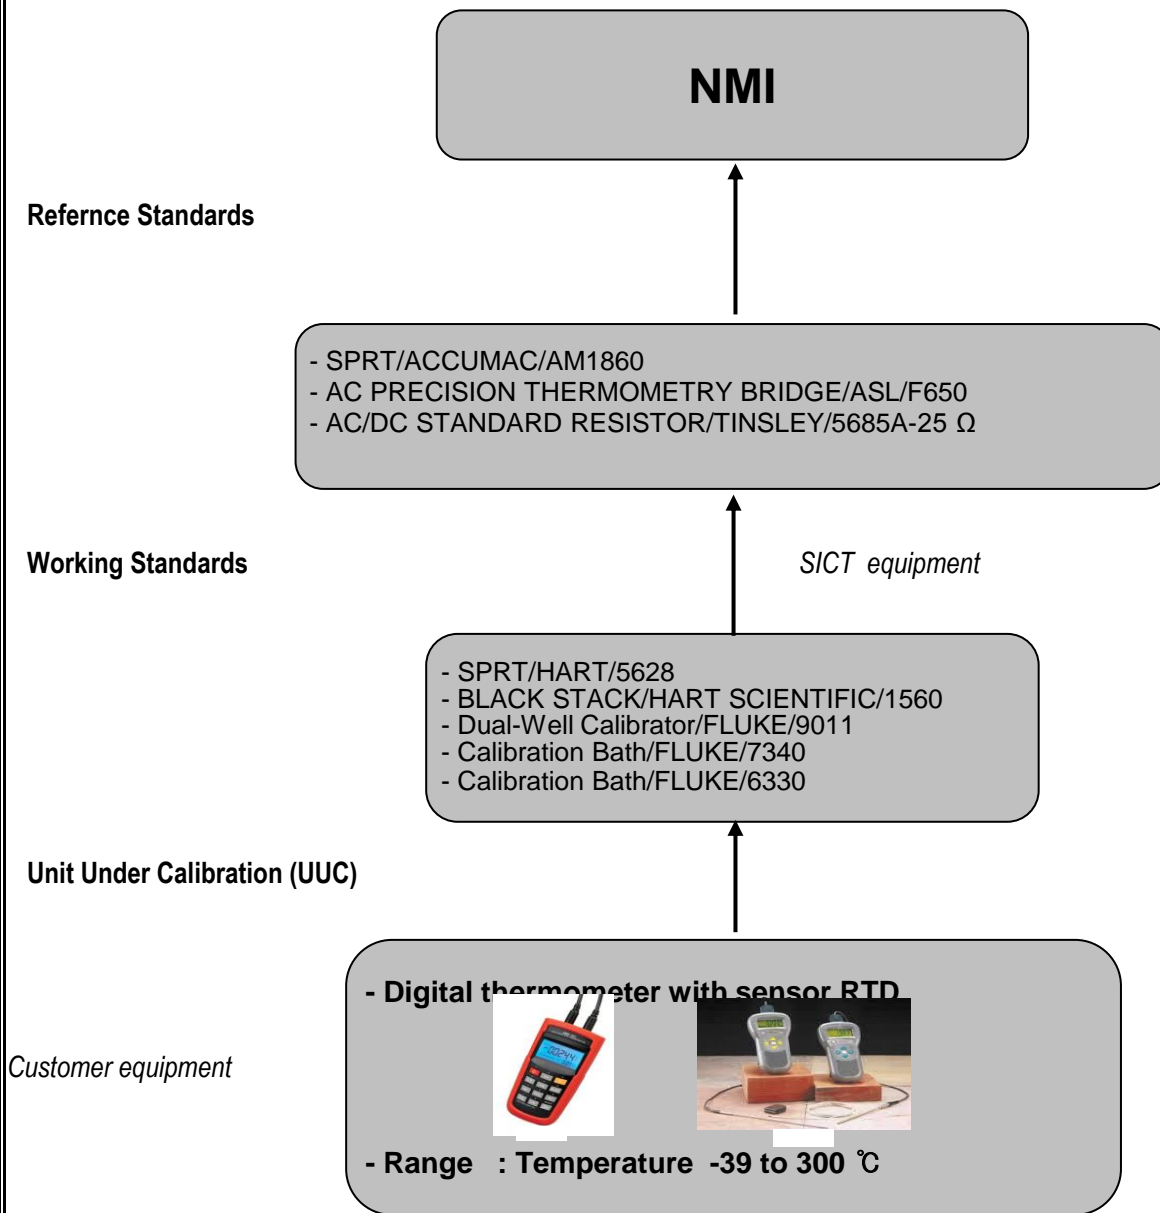

Remark :

- NMI : National Metrology Institute
- KRISS : Korea Research Institute of Standard and Science (Republic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd.