


# Traceability Chart

|                      |                     |                               |
|----------------------|---------------------|-------------------------------|
| หมายเลขเอกสาร :      |                     | แก้ไขที่ : 0                  |
| DRAF<br><i>Pawit</i> | CHECK<br><i>TL.</i> | APPROVE<br><i>[Signature]</i> |
| Date :               | Date :              | Date :                        |

Name of Laboratory : Thai-Korea Calibration Center Co.,Ltd. (TKCC)  
 Accreditation No. : Accredited by TLAS Calibration No. 0116  
 Calibration procedure : WL-E046 Temperature transducers  
 Calibration scope for : Temperature -40 °C to 500 °C

## Traceable to National Metrology Institute (NMI)

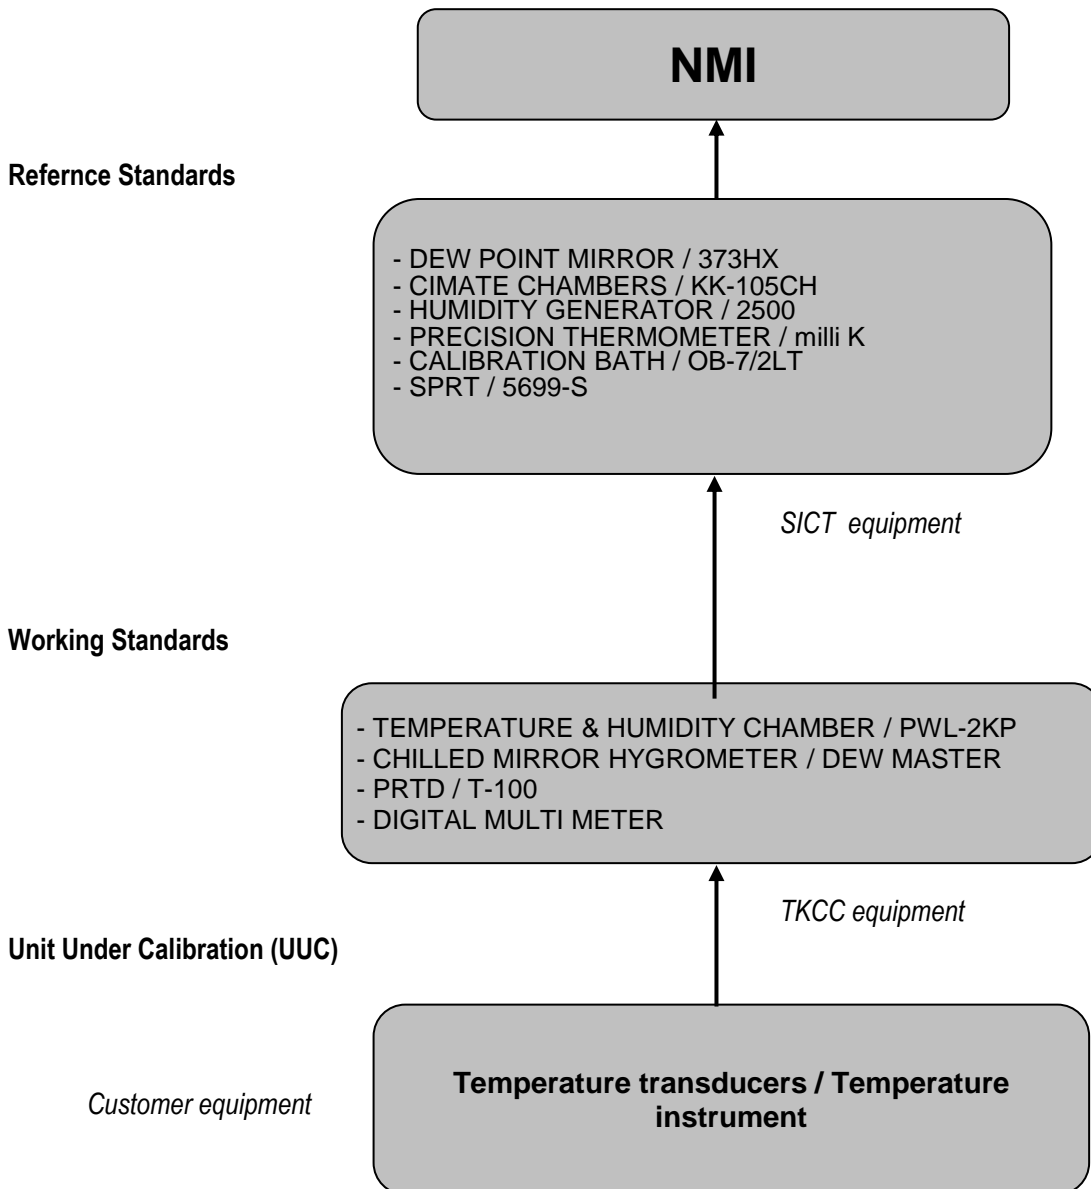

Remark :

- NMI : National Metrology Institute
- KRISS : Korea Research Institute of Standard and Science (Republic of Korea)
- NIMT : National Institute of Metrology (Thailand)
- SICT : Institute of Calibration & Technology Co.,Ltd.